
















COMPARATIVE STATEMENT FOR SURGICAL DISPOSABLE /MEDICAL DEVICES (A013).





T.E. No	Product Name	Specification	Name of Bidder	Technical Status (Responsive/ Non-Responsive) In case of failure mention reason of rejection		Sample status (Responsive/ Non-responsive) In case of failure mention reason of rejection	Final Recommendation
				PART A	PART B	PART C	
1	Bladder Wash Syringe 60cc	Single sterile blister pack capacity 60mL with catheter tip latex free	Adnan	Responsive	Responsive	Responsive	Responsive
2	Disp. Syringe 5cc AD	Auto-disable 5mL capacity 23G needle, single sterile in blister pack.	Care & Cure	Responsive	Responsive	Responsive	Responsive
			Mediserve	Responsive	Responsive	Responsive	Responsive
			K.M.Enter	Non-Responsive Firm is Blacklisted till 2032	Responsive	Responsive	Non-Responsive. Firm is Blacklisted till 2032
			Medicare	Responsive	Responsive	Responsive	Responsive






			Fatima Traders	Non-Responsive Invalid CDR or Bank guarantee	Responsive	Responsive	Non-Responsive Invalid CDR or Bank guarantee
			Adnan	Responsive	Responsive	Responsive	Responsive
3	Disp. Syringe 10cc	10mL capacity 21G needle, single sterile in blister pack.	Care & Cure	Responsive	Responsive	Responsive	Responsive
			Mediserve	Responsive	Responsive	Responsive	Responsive
			K.M.Enter	Non-Responsive Firm is Blacklisted till 2032	Responsive	Responsive	Non-Responsive Firm is Blacklisted till 2032
			Fatima Traders	Non-Responsive Invalid CDR or Bank guarantee	Responsive	Responsive	Non-Responsive Invalid CDR or Bank guarantee
			Adnan	Responsive	Responsive	Responsive	Responsive
4	Disp. Syringe 20cc	20mL capacity 21G needle, single sterile in blister pack.	K.M.Enter	Non-Responsive Firm is Blacklisted till 2032	Responsive	Responsive	Non-Responsive Firm is Blacklisted till 2032
			Adnan	Responsive	Responsive	Responsive	Responsive

5	Disp. Syringe 1cc AD	Auto-disable 1mL capacity, 25G needle and 1"length, single	Mediserve	Responsive	Responsive	Responsive	Responsive
6	Disp. Syringe 50 cc	50mL capacity 21G needle, single sterile in blister pack.	Adnan	Responsive	Responsive	Responsive	Responsive
7	Disp. Insulin Syringe	Capacity, 29- 30G needle and 0.5"length, single sterile in blister pack.	K.M.Enter	Non- Responsive Firm is Blacklisted till 2032	Responsive	Responsive	Non-Responsive Firm is Blacklisted till 2032
			Ashal	Non- Responsive Invalid CDR or Bank guarantee	Responsive	Responsive	Non-Responsive Invalid CDR or Bank guarantee
			Adnan	Responsive	Responsive	Responsive	Responsive
8	IV Canula 18G	1.3x45±2mm, 90±10mL/min,	The Searle	Responsive	Responsive	Responsive	Responsive
			Mediserve	Responsive	Responsive	Responsive	Responsive

		single sterile in blister pack with colour coding	Lab-link	Non-Responsive Specifications are in correct 1.3 *32mm rather than 1.3*45mm	Responsive	Non-Responsive Specifications are in correct 1.3 *32mm rather than 1.3*45mm	Non-Responsive Specifications are in correct 1.3 *32mm rather than 1.3*45mm
			K.M.Enter	Non-Responsive Firm is Blacklisted till 2032	Responsive	Responsive	Non-Responsive Firm is Blacklisted till 2032
			Medicare	Responsive	Responsive	Responsive	Responsive
			Ashal	Non-Responsive Invalid CDR or Bank guarantee	Responsive	Responsive	Non-Responsive Invalid CDR or Bank guarantee
			Adnan	Non-Responsive specifications are not mentioned on label of the product	Responsive	Non-Responsive Required specifications are not mentioned on label of the product	Non-Responsive Required specifications are not mentioned on label of the product
9	IV Canula 20G	1.1x33±2mm, 60±10mL/min, sterile in blister	The Searle	Responsive	Responsive	Responsive	Responsive
			Mediserve	Responsive	Responsive	Responsive	Responsive

		pack with colour coding	Lab-link	Responsive	Responsive	Responsive	Responsive
			K.M.Enter	Non-Responsive Firm is Blacklisted till 2032	Responsive	Responsive	Non-Responsive Firm is Blacklisted till 2032
			Medicare	Responsive	Responsive	Responsive	Responsive
			Ashal	Non-Responsive Invalid CDR or Bank guarantee	Responsive	Responsive	Non-Responsive Invalid CDR or Bank guarantee
			Adnan	Non-Responsive Specifications are not mentioned on label of the product	Responsive	Non-Responsive Required specifications are not mentioned on label of the product	Non-Responsive Required specifications are not mentioned on label of the product
10	IV Canula 22G	0.9x25±2mm, 36±10mL/min, single sterile in blister pack with colour coding	The Searle	Responsive	Responsive	Responsive	Responsive
			Mediserve	Responsive	Responsive	Responsive	Responsive
			Lab-link	Responsive	Responsive	Responsive	Responsive
			K.M.Enter	Non-Responsive Firm is Blacklisted till 2032	Responsive	Responsive	Non-Responsive Firm is Blacklisted till 2032

As per

of A

			Medicare	Responsive	Responsive	Responsive	Responsive
			Ashal	Non-Responsive Invalid CDR or Bank guarantee	Responsive	Responsive	Non-Responsive Invalid CDR or Bank guarantee
			Adnan	Non-Responsive Specifications are not mentioned on label of the product	Responsive	Non-Responsive Required specifications are not mentioned on label of the product	Non-Responsive Required specifications are not mentioned on label of the product
11	IV Canula 24G with inj port	0.7x 19±2mm, 20±10mL/min, single sterile in blister pack	The Searle	Responsive	Responsive	Responsive	Responsive
			Mediserve	Responsive	Responsive	Responsive	Responsive
			Lab-link	Responsive	Responsive	Responsive	Responsive
			K.M.Enter	Non-Responsive Firm is Blacklisted till 2032	Responsive	Responsive	Non-Responsive Firm is Blacklisted till 2032
			Medicare	Responsive	Responsive	Responsive	Responsive
			Ashal	Non-Responsive	Responsive	Responsive	Non-Responsive

Dr. Min

FA

[Signature]


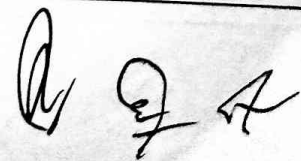
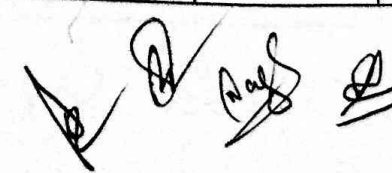
[Signature]

[Signature]







				Invalid CDR or Bank guarantee			Invalid CDR or Bank guarantee
			Adnan	Non-Responsive Specifications are not mentioned on label of the product	Responsive	Non-Responsive Required specifications are not mentioned on label of the product	Non-Responsive Required specifications are not mentioned on label of the product
12	Latex Examination Gloves 1x100	powdered gloves fit in either hand with high elasticity with minimum wt 5gm/glove	Eastern	Responsive	Responsive	Responsive	Responsive
			Care & Cure	Responsive	Responsive	Responsive	Responsive
			K.M.Enter	Non-Responsive Firm is Blacklisted till 2032	Responsive	Responsive	Non-Responsive Firm is Blacklisted till 2032
			Clifton	Responsive	Responsive	Responsive	Responsive
13	Micro-Burette	volumetric chamber for infusion 100mL with set made of PVC Tube, min. length 150cm, registered with DRAP	Care & Cure	Responsive	Responsive	Responsive	Responsive
			Roy & Roy's	Responsive	Responsive	Responsive	Responsive
			PMS	Non-Responsive Invalid CDR or Bank guarantee.	Non-Responsive (Passing Marks are	Responsive	Non-Responsive Invalid CDR or Bank guarantee. Affidavit of the sole agent is

[Handwritten signatures and initials]






				Affidavit of the sole agent is Submitted by name of PMS but firm name is written as "Roy and Roy's" in statement lines	not obtained)		Submitted by name of PMS but firm name is written as "Roy and Roy's" in statement lines
			K.M.Enter	Non-Responsive Firm is Blacklisted till 2032	Responsive	Responsive	Non-Responsive Firm is Blacklisted till 2032
14	Surgical Gloves 6.5	Sterile single pack glove pair with/without powder and thickness as per ISO 10282. Pack size fifty pair per pack	Eastern	Non-Responsive ISO 10282 is not mentioned on Label of product	Responsive	Non-Responsive ISO 10282 is not mentioned on Label of product	Non-Responsive ISO 10282 is not mentioned on Label of product
			The Searle	Non-Responsive ISO 10282 is not mentioned on Label of product	Responsive	Non-Responsive ISO 10282 is not mentioned on Label of product	Non-Responsive ISO 10282 is not mentioned on Label of product








			Mediserve	Responsive	Responsive	Responsive	Responsive
			Medicare	Non-Responsive Valid quality certificate is not attached and ISO 10282 is not mentioned on Label of product	Responsive	Non-Responsive ISO 10282 is not mentioned on Label of product	Non-Responsive Valid quality certificate is not attached and ISO 10282 is not mentioned on Label of product
			Clifton	Responsive	Responsive	Responsive	Responsive
			Adnan	Non-Responsive ISO 10282 is not mentioned on Label of product	Responsive	Non-Responsive ISO 10282 is not mentioned on Label of product	Non-Responsive ISO 10282 is not mentioned on Label of product
15	Surgical Gloves 7.0	Sterile single pack glove pair with/without powder and thickness as per ISO 10282.	Eastern	Non-Responsive ISO 10282 is not mentioned on Label of product	Responsive	Non-Responsive ISO 10282 is not mentioned on Label of product	Non-Responsive ISO 10282 is not mentioned on Label of product
			The Searle	Non-Responsive ISO 10282 is not mentioned	Responsive	Non-Responsive ISO 10282 is not mentioned on Label of product	Non-Responsive ISO 10282 is not mentioned on Label of product







				on Label of product			
			Mediserve	Responsive	Responsive	Responsive	Responsive
			Medicare	Non-Responsive Valid quality certificate is not attached and ISO 10282 is not mentioned on Label of product	Responsive	Non-Responsive ISO 10282 is not mentioned on Label of product	Non-Responsive Valid quality certificate is not attached and ISO 10282 is not mentioned on Label of product
			Clifton	Responsive	Responsive	Responsive	Responsive
			Adnan	Non-Responsive ISO 10282 is not mentioned on Label of product	Responsive	Responsive ISO 10282 is not mentioned on Label of product	Non-Responsive ISO 10282 is not mentioned on Label of product
16	Surgical Gloves 7.5	Sterile single pack glove pair with/without powder and thickness as per ISO 10282. Pack size fifty pair per pack	Eastern	Non-Responsive ISO 10282 is not mentioned on Label of product	Responsive	Non-Responsive ISO 10282 is not mentioned on Label of product	Non-Responsive ISO 10282 is not mentioned on Label of product
			The Searle	Non-Responsive	Responsive	Non-Responsive	Non-Responsive


				ISO 10282 is not mentioned on Label of product		ISO 10282 is not mentioned on Label of product	ISO 10282 is not mentioned on Label of product
			Mediserve	Responsive	Responsive	Responsive	Responsive
			Medicare	Non-Responsive Valid quality certificate is not attached and ISO 10282 is not mentioned on Label of product	Responsive	Non-Responsive ISO 10282 is not mentioned on Label of product	Non-Responsive Valid quality certificate is not attached and ISO 10282 is not mentioned on Label of product
			Clifton	Responsive	Responsive	Responsive	Responsive
			Adnan	Non-Responsive ISO 10282 is not mentioned on Label of product	Responsive	Non-Responsive ISO 10282 is not mentioned on Label of product	Non-Responsive ISO 10282 is not mentioned on Label of product
17	Surgical Gloves 8.0	Sterile single pack glove pair with/without powder and thickness as per ISO 10282. Pack	Eastern	Non-Responsive ISO 10282 is not mentioned on Label of product	Responsive	Non-Responsive ISO 10282 is not mentioned on Label of product	Non-Responsive ISO 10282 is not mentioned on Label of product











		size fifty pair per pack	The Searle	Non-Responsive ISO 10282 is not mentioned on Label of product	Responsive	Non-Responsive ISO 10282 is not mentioned on Label of product	Non-Responsive ISO 10282 is not mentioned on Label of product
			Mediserve	Responsive	Responsive	Responsive	Responsive
			Medicare	Non-Responsive Valid quality certificate is not attached and ISO 10282 is not mentioned on Label of product	Responsive	Non-Responsive ISO 10282 is not mentioned on Label of product	Non-Responsive Valid quality certificate is not attached and ISO 10282 is not mentioned on Label of product
			Clifton	Responsive	Responsive	Responsive	Responsive
			Adnan	Non-Responsive ISO 10282 is not mentioned on Label of product	Responsive	Non-Responsive ISO 10282 is not mentioned on Label of product	Non-Responsive ISO 10282 is not mentioned on Label of product
18	Scalp Needle Sizes	Vein All	Lab-link	Non-Responsive Valid Quality certificate is attached of	Responsive	Responsive	Non-Responsive Valid Quality certificate is attached of Japan, not of Thailand










		luer lock sterile single pack		Japan, not of Thailand			
--	--	----------------------------------	--	---------------------------	--	--	--



Dr. Aftab Ahmad
SMO Anesthesia
(Member)



Dr. Shahbaz Ahmad
Medical Officer/ AMS (H)
(Member)



Ms. Naghmana
Deputy Drug Controller
(Member)


Ms. Shazia Khanam
Deputy Drug Controller
(Member)


Ms. Shabnam Akram
Hospital Pharmacist
(Member)


Mr. Zuhair Mehdi
Hospital Pharmacist
(Member)


Ms. Sana Ijaz
Hospital Pharmacist
(Member)


Prof. Dr. Muhammad Iqbal Mirza
Head of Orthopedic Unit I
(Chairman T.E)